


## Isocratic Analysis of the Alcohols Present in a Generic Hand/Spray Sanitizer on Orosil C18-HC, 3 $\mu$ m

Use: Various uses

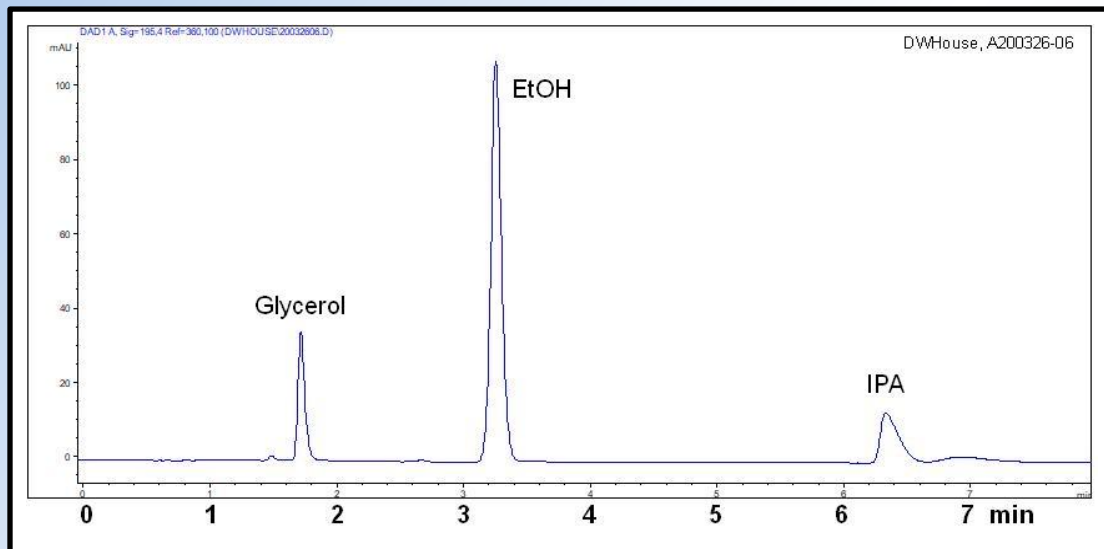

<b>UHPLC</b>	Agilent 1100	<b>Glycerol, R<sub>1</sub></b>	1.72 min
<b>Column</b>	Orosil C18-HC, 3 microns	<b>Ethanol, R<sub>2</sub></b>	3.25 min
<b>Column Size</b>	4.6 mm ID x 150 mm long	<b>2-Propanol (IPA), R<sub>3</sub></b>	6.33 min
<b>Temperature</b>	25 °C		
<b>Detection</b>	UV at 195 nm		
<b>Injection</b>	25 $\mu$ L		
<b>Mobile Phase Isocratic</b>	A: 2% Acetonitrile B: 98% Water		
<b>Flow Rate</b>	1.0 mL/min		