


Separation of Bucetin on Epitomize CSP-1A by UHPLC

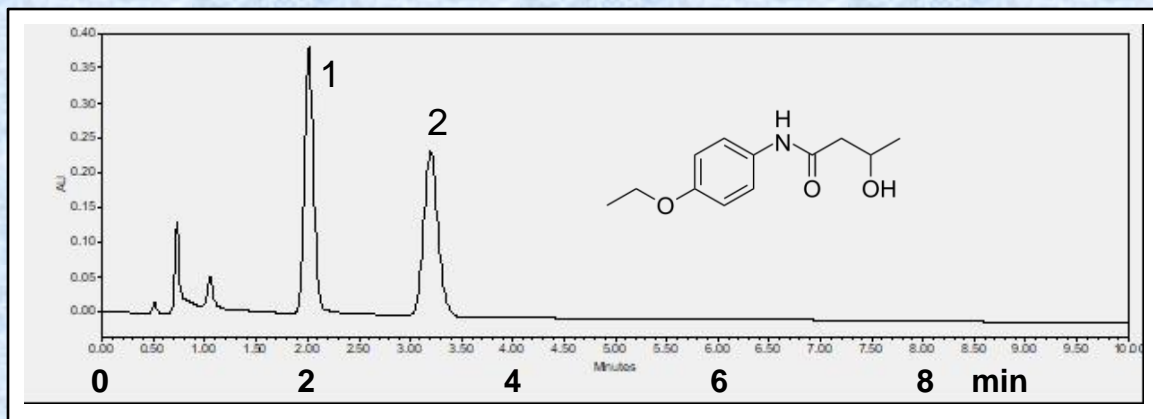

Sample	Bucetin [D21639]		
System	Waters Acquity, H-Class		
Column	Epitomize CSP-1A, 3 micron, 3.0 x 50 mm		
Mobile Phase	80/20/0.1 Heptane/2-propanol/diethylamine		
Flow Rate	0.50 mL/min	Rt1 & Rt2 (min)	2.01 & 3.20
Temperature	25 °C	k1 & k2	3.25 & 5.75
Detection	UV at 254 nm	Separation Value	1.77
Injection	0.50 µL (1 mg/mL)	Resolution	5.75