# Chiral Applications Library

Application Note: UCEP-1K-18102

## Separation of Flavanone on Epitomize CSP-1K by UHPLC

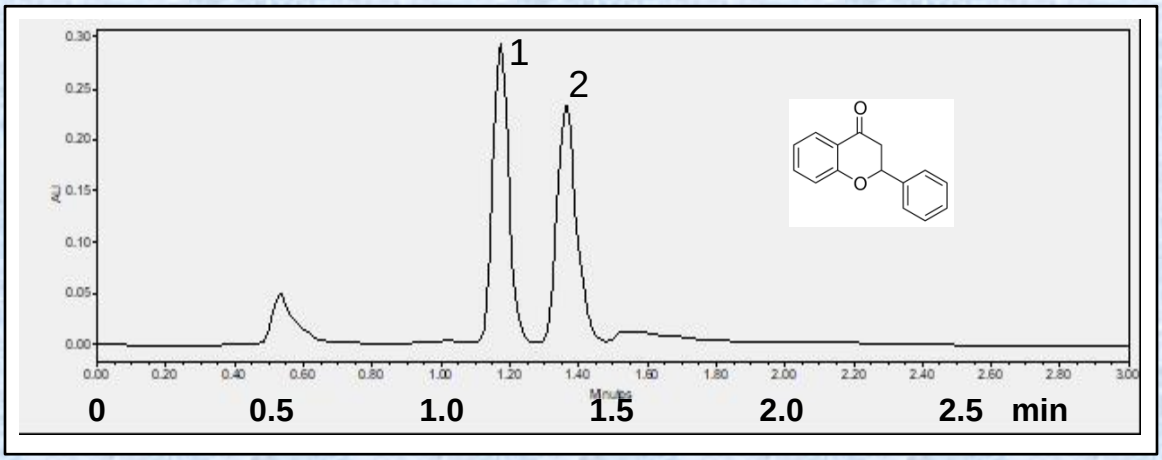


| | | | |
|---|---|---|---|
| **Sample** | Flavanone [D25733] | | |
| **System** | Waters Acquity, H-Class | | |
| **Column** | Epitomize CSP-1K, 3 micron, 3.0 x 50 mm | | |
| **Mobile Phase** | 80/20 Heptane/2-propanol | | |
| **Flow Rate** | 0.50 mL/min | **Rt1 & Rt2 (min)** | 1.17 & 1.36 |
| **Temperature** | 25 °C | **k1 & k2** | 1.29 & 1.66 |
| **Detection** | UV at 230 nm | **Separation Value** | 1.29 |
| **Injection** | 0.50 µL (1 mg/mL) | **Resolution** | 2.03 |

Orochem Technologies Inc
340 Shuman Blvd.
Naperville, IL 60563

Tel.: 630-210-8300
Fax: 630-210-83150250
www.orochem.com