


Separation of Warfarin on Epitomize CSP-1Z by UHPLC

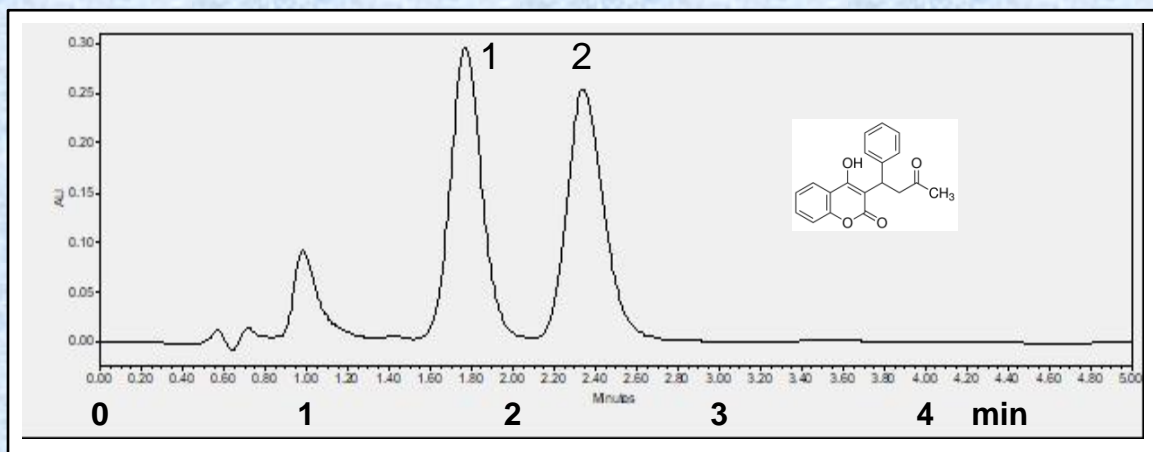

| | | | |
|---------------------|-----------------------------------------|----------------------------|-------------|
| Sample | Warfarin [D20767] | | |
| System | Waters Acquity, H-Class | | |
| Column | Epitomize CSP-1Z, 3 micron, 3.0 x 50 mm | | |
| Mobile Phase | 80/20/0.1 Heptane/2-propanol/TFA | | |
| Flow Rate | 0.50 mL/min | Rt1 & Rt2 (min) | 1.77 & 2.34 |
| Temperature | 25 °C | k1 & k2 | 2.43 & 3.54 |
| Detection | UV at 210 nm | Separation Value | 1.45 |
| Injection | 0.50 µL (1 mg/mL) | Resolution | 1.92 |